

Syphilis (anti-tp), Blood-Based Home Test (Tri-line) Test Cassette Manual

Home Screening Test for Syphilis (bacteria Treponema Pallidum).



- One individual sealed pouch containing
- Test device
- Alcohol pad
- Instructions

Material Required but not provided

- Time or Watch capable of timing 10 to 30 minutes
- Clean, Disposable, Absorbent Workspace Cover
- Biohazard Waste Container

PRECAUTIONS


- Carefully follow the instructions exactly.
- Only use the included pipette.
- This kit is for in vitro use only. Do not swallow.
- Contaminated blood may cause erroneous results.
- Discard after first use. The test can only be used once.
- Do not use test kit beyond the expiration date.
- Do not use the kit if the pouch is punctured or not well sealed.
- Keep out of children's reach.

STORAGE AND STABILITY

- Store at 4°C to 30°C in the sealed pouch up to expiration date.
- Keep away from sunlight, moisture and heat.
- Use the test shortly after opening the pouch.
- Do not freeze.

TEST PROCEDURE

- When the test has been stored in a cold room, wait for it to reach room temperature (10°C - 30°C).
- Wash the hands thoroughly to avoid contamination of the specimen.
- Open the pouch and place the cassette on a level surface.
- Clean the area to be lanced with the alcohol pad.
- Wait for the area to dry completely (do not blow on it).
- Use the safety lancet and pipette. The safety lancet can only be used once.

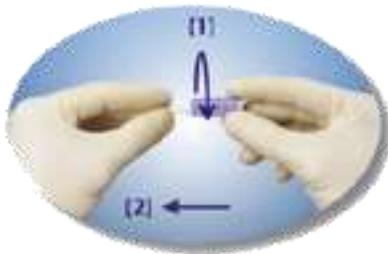

Twist off the protective cap, and then pull it straight out.




Press the lancet firmly against the puncture site to activate the device.



Gently apply intermittent pressure near the puncture site to obtain the required blood volume

- Squeeze the pipette together and collect blood by slowly releasing the pressure.
- Add 1-2 drop of blood, from the pipette, to the round well of the cassette.
- If the blood sample is not moving across the membrane within one minute, add one more drop of blood sample to the round well of the cassette.

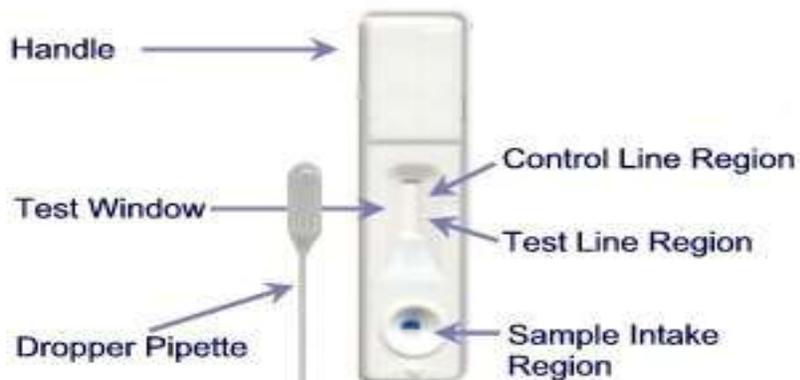

HOW TO INTERPRET THE RESULT

Read the result 15 minutes after adding the blood sample. Do not read the result after 20 minutes.

Positive Syphilis "Bacteria Treponema Pallidum" infection:

Colored lines are visible in the control region and the test region. This means that infection by Syphilis (Bacteria Treponema Pallidum) is likely, it needs to be confirmed with a secondary test before it is diagnosis and treated.

The intensity of the color of the lines varies due to different concentrations of Syphilis antibodies but also other blood values and therefore no meaning is attributed to line color intensity or width.

Negative No Syphilis "Bacteria Treponema Pallidum" infection:

One colored line is visible in the control region and no colored line in the test region. This means that no Syphilis (Bacteria Treponema Pallidum) infection was detected.

Invalid:

There are no colored lines or only a colored line in the test region. The most common reason for an invalid test result is that the test procedure was not carried out properly.

